


HPLC REPORT

Sample Name:	VE-822	Injection Volume:	10.0
Vial Number:	RA3	Channel:	UV_VIS_4
Sample Type:	unknown	Wavelength:	254
Control Program:		Bandwidth:	4
Quantif. Method:	default	Dilution Factor:	1.0000
Recording Time:	2015/4/23 11:58	Sample Weight:	1.0000
Run Time (min):	12.66	Sample Amount:	1.0000

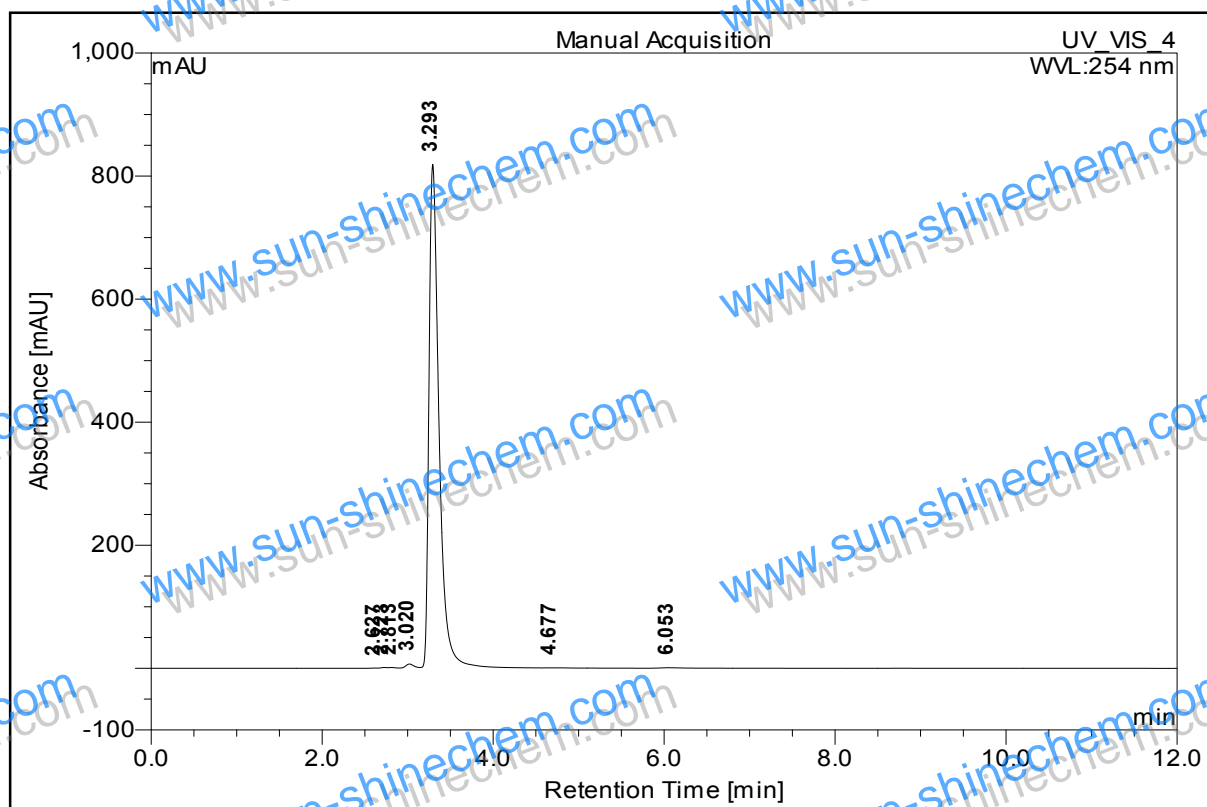

No.	Ret. Time min	Peak Name	Height mAU	Area mAU*min	Rel.Area %	Amount n.a.	Type
1	2.63	n.a.	0.121	0.010	0.01	n.a.	Ru
2	2.72	n.a.	1.232	0.125	0.11	n.a.	BM
3	2.81	n.a.	1.164	0.108	0.10	n.a.	M
4	3.02	n.a.	6.784	0.773	0.68	n.a.	M
5	3.29	n.a.	818.606	111.812	98.82	n.a.	Mb*
6	4.68	n.a.	0.176	0.051	0.05	n.a.	bMB
7	6.05	n.a.	0.764	0.265	0.23	n.a.	BMB*
Total:			828.847	113.144	100.00	0.000	